

PneumoDart®

REF TM-317 For Single Use Only

14 ga x 3.25 in. NSN 6515-01-655-9514

TyTek Medical Inc.

8904 Beckett Rd, West Chester, OH 45069

www.tytekmedical.com



Emergo Europe
Prinsessegracht 20
2514 AP The Hague
The Netherlands
Tel: (+31) 70 345 8570
Fax: (+31) 70 346 7299

STERILE R

CE
1639

tytek
medical
(+1) 513-247-2002

Instructions For Trained Medical Personnel

- Select the location for the needle to enter by identifying the second intercostal space on the anterior chest at the mid-clavicular line on the same side of the body as the injury. (FIG. 1)
- Use antimicrobial solution to cleanse the needle-insertion site.
- Inspect that the safety seal is intact. If not intact, do not use the product. With a firm grip on the PneumoDart®, twist the hex cap to break the seal, and remove the cap.
- Remove the PneumoDart® needle from its case.
- Insert the needle assembly into the patient's skin over the superior border of the third rib at the mid-clavicular line. Direct the needle into the intercostal space at a 90° angle to the chest wall, being careful that the entry is not medial to the nipple line and not directed toward the heart.
- Spring-loaded, retractable safety tip (FIG 3) retracts as the needle is pushed through the chest wall and automatically advances once the pleural cavity is penetrated, if a pneumothorax is present.
- Visual Needle Position Indicator (FIG 4). Once the PneumoDart® penetrates pleural cavity, the green indicator will click in the down position and you will hear a sudden escape of air as the tension pneumothorax is decompressed.
- Secure in a manner directed by your training.
- Monitor the patient carefully for any tension pneumothorax recurrences or respiratory distress.

MIDCLAVICULAR
SECOND INTERCOSTAL
SPACE

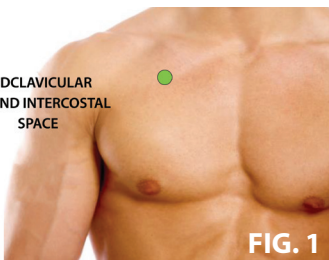


FIG. 1



FIG. 2



FIG. 3

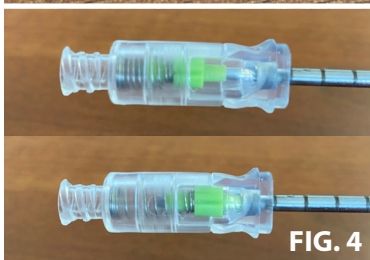


FIG. 4

Body Substance Isolation Alert

Always use appropriate body substance isolation procedures and personal protective equipment in order to prevent contact with contaminated fluids.

Caution

PneumoDart® should only be used by personnel who have received proper training on procedures for relieving a tension pneumothorax with this device. Improper use of PneumoDart® could cause injury. Use PneumoDart® as directed by your EMS authority or by a physician. Do not place PneumoDart during active chest compressions.

Potential hazards of needle decompression include cardiac tamponade, life-threatening bleeding due to pulmonary artery, aorta or intercostal vessel injury, non-therapeutic insertion and potential nerve injury at insertion site. Hazards can be avoided by adhering to approved protocols, training and site placement. Failure to adhere may result in patient decompensation, injury and/or death.

PneumoDart®

NSN: 6515-01-541-0635 14 ga x 3.25 in.

STERILE | R

For Single Use Only

CE
1639

REF TM-317



Emergo Europe
Prinsessegracht 20
2514 AP The Hague
The Netherlands
Tel: (+31) 70 345 8570
Fax: (+31) 70 346 7299

TyTek Medical Inc.

www.tytekmedical.com | 8904 Beckett Rd, West Chester, OH 45069

Disposal

PneumoDart® is for single-use only. It is not re-usable under any circumstances. It may be used once, and then must be properly disposed. Dispose of PneumoDart® in a way that assures body substance isolation of potentially infectious substances and prevents sharps injury.

Storage

Keep PneumoDart® dry, stored in temperatures between 10°F and 140°F.

Limited Warranty

The products and components contained in this package are medical devices intended solely for use by appropriately trained healthcare professionals. TyTek Medical Inc. warrants that the products and components are free from defects in material and workmanship and fit solely for use as medical devices for the specific purpose described in the manual by trained healthcare professionals for a period of 12 months from the date of shipment by TyTek Medical Inc. Any use of the products or components beyond the specific use described in this manual or by a person not trained or legally authorized to use the products or components voids this limited warranty. EXCEPT AS SET FORTH HEREIN, TYTEK MEDICAL INC. MAKES NO OTHER WARRANTIES, EXPRESS OR IMPLIED, REGARDING THE PRODUCTS OR COMPONENTS AND SPECIFICALLY DISCLAIMS THE IMPLIED WARRANTIES OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE.

This item sold and to be used strictly per terms and conditions at www.tytekmedical.com.

